

QR Code Will
Appear Here

SmartExam: ON

Demo

M

Demo

Demo

Height:

Weight:


Physician:

Others

Fasting:

CAP (dB/m)		E (kPa)	
SD	MEAN	MEDIAN	IQR/Med
16	377	5.7	12%

Demo Exam: XL
SWF = 50Hz
Organ: Liver
Operator: vishnu
E-MEASUREMENTS: 10
CAP-LEVEL: >100 %

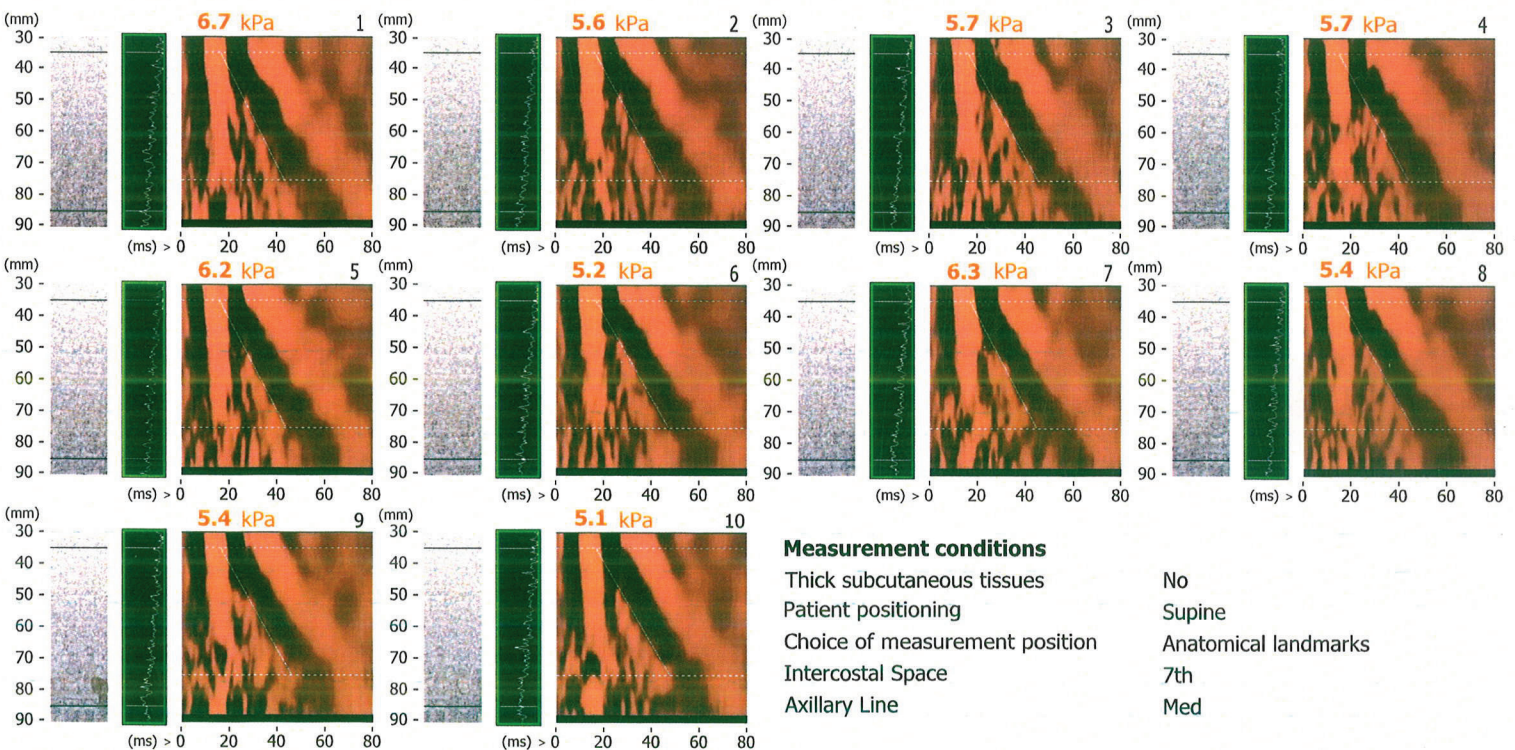

FibroScan 430 Mini + / SN: F96467

Probe XL+ / SN: 2008806

Software release number FS 4.1.5

FibroScan® is a medical device intended as an aid for the management of patients with liver disease. Measurements should be performed by a certified operator. The values obtained must be interpreted by a physician experienced in dealing with liver disease, taking into account the complete medical records of the patient, the number of valid measurements and their dispersion. Probes must be calibrated according to the manufacturer's recommendations.